



FAME of olive oil

Application Note

Food Testing & Agriculture

Authors

Agilent Technologies, Inc.

Introduction

The low bleed Agilent FactorFour VF-23ms delivers fast GC separation of FAME isomers from olive oil within five minutes.



Agilent Technologies


Conditions

Technique : GC
Column : Agilent VF-23ms, 0.25 mm x 30 m fused silica
(df = 0.25 μ m) (Part no. CP8822)
Temperature : 185 °C
Carrier Gas : Hydrogen, 70 kPa
Injector : Split, 1:100
T = 275 °C
Detector : FID
Sample Size : 0.5 μ L
Concentration Range : ca. 5 ng per component on the column

Courtesy : J. Peene, Agilent R&D laboratories, Middelburg,
The Netherlands

Peak identification

1. C16:0
2. C16:1 9-cis
3. C18:0
4. C18:1 9-cis
5. C18:2 9-cis, 12-cis
6. C18:3 9-cis, 12-trans, 15-cis
7. C18:3 9-cis, 12-cis, 15-cis

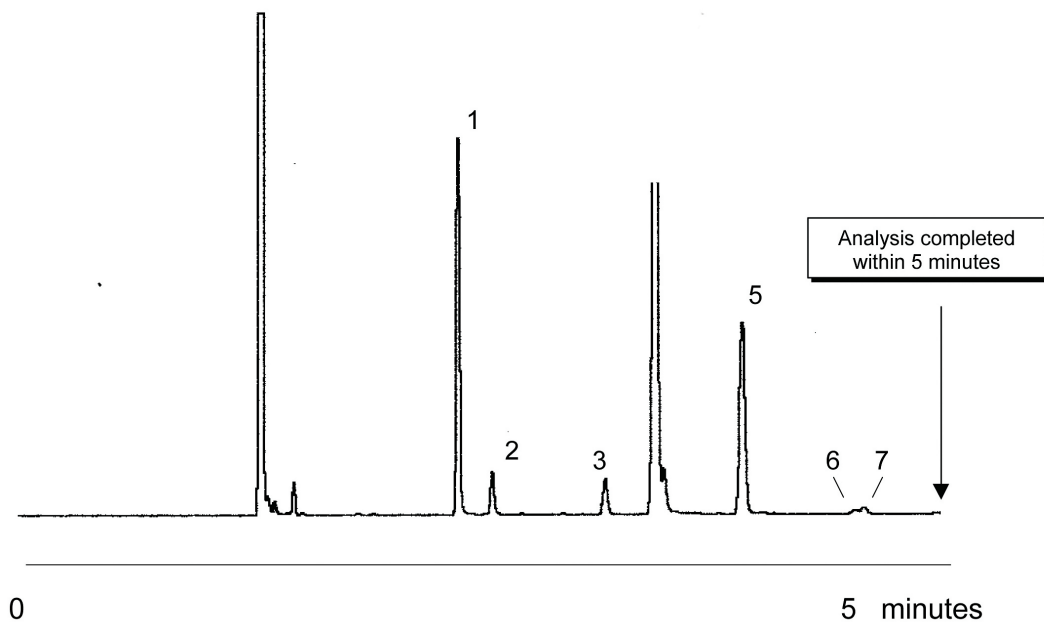

www.agilent.com/chem

This information is subject to change without notice.

© Agilent Technologies, Inc. 2011

Printed in the USA

31 October, 2011

First published prior to 11 May, 2010

A01975



Agilent Technologies