

# Separation of Acidic and Neutral Drugs Using a Core Enhanced Technology Accucore HPLC Column

Anila Khan, Thermo Fisher Scientific, Runcorn, Cheshire, UK

## Abstract

This application note demonstrates the use of the Thermo Scientific Accucore C18 column for the separation of acidic and neutral drugs.

## Introduction

Therapeutic monitoring of drugs is very important in the pharmaceutical industries as compliance with the FDA regulations is required. Chromatography of acidic drugs can be problematic as they can exhibit peak tailing due to interaction with active sites on the stationary phase of column. Accucore™ HPLC columns use Core Enhanced Technology to facilitate fast and high efficiency separations. The 2.6 µm diameter particles are not totally porous, but rather have a solid core and a porous outer layer. The optimised phase bonding creates a series of high coverage, robust phases. The carbon loading of Accucore C18 provides high retention of non-polar analytes via a predominantly hydrophobic interaction mechanism, enabling the separation of a broad range of analytes. The tightly controlled 2.6 µm diameter of Accucore particles results in much lower backpressures than typically seen with sub-2 µm materials. These columns have shown to give an excellent peak shapes for acidic and neutral drugs in acidic conditions.



## Sample Preparation

A 1000 µg/mL mixture of acidic and neutral drugs (listed in Table 1) was prepared in 1:1 Far UV Acetonitrile/water; this solution was then diluted in water to the required concentration for analysis (stated in Table 1)

Thermo Scientific Column	Part Number
Accucore C18 2.6 µm 100 x 2.1 mm	17126-102130
Measured backpressure: 256 bar	

## Thermo Scientific Accela HPLC/UHPLC

Column temperature	25 °C
Injection volume	1.5 µL
Flow rate	0.40 mL/min
PDA/UV detection	215 nm

## Mobile Phase

A: 0.1% Phosphoric acid Water

B: 0.1% Phosphoric acid Far UV Acetonitrile

Gradient:

Time/min	A	B
0	70	30
2	60	40
4	5	95
8	5	95

Consumables	Part Number
Fisher Scientific HPLC grade water	W/0106/17
Fisher Scientific HPLC grade Far UV acetonitrile	268260025
HPLC grade phosphoric acid, Fisher Scientific	0/0515/PB08
Liquid handling hardware: FinnPipette (100-1000 µL)	642090
NSC Mass Spec Certified 2 mL clear vial with PTFE silicone cap	MSCERT4000-34W

## Key Words

- Accucore C18
- Superficially porous
- Core Enhanced Technology
- Acidic and neutral drugs
- Fused core

## Results

Figure 1 shows the chromatogram of acidic and neutral drugs separated on an Accucore C18 2.6 µm 100 x 2.1 mm column. The analysis demonstrates this column can provide not only a good baseline resolution but excellent retention time reproducibility when these drugs are separated.

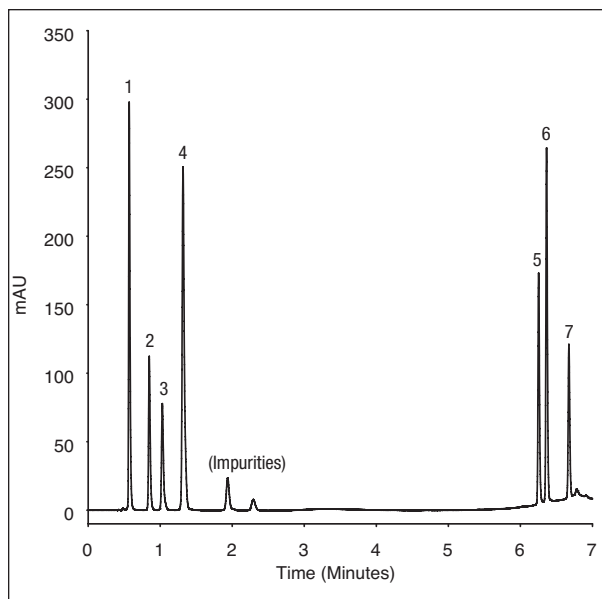


Figure 1: Chromatogram of acidic and neutral drugs separated on an Accucore C18 2.6 µm 100 x 2.1 mm column

	Compounds	Sample Concentration (µg/mL)	t <sub>r</sub> /min	%RSD (t <sub>r</sub> /min) n=6
1	Hydrochlorothiazide	20	0.57	0.13
2	Prednisolone	50	0.85	0.19
3	Pravastatin	50	1.03	0.27
4	Carbamazepine	20	1.32	0.20
5	Diclofenac	20	6.29	0.59
6	Ibuprofen	50	6.40	0.57
7	Progesterone	50	6.71	0.54

Table 1: The analysis of acidic and neutral drugs on an Accucore C18 2.6 µm 100 x 2.1 mm column

## Conclusions

The separation of acidic and neutral drugs was successfully achieved on Accucore C18 column, providing an excellent choice for the analysis of these drugs giving excellent retention time reproducibility and resolution.

*In addition to these offices, Thermo Fisher Scientific maintains a network of representative organizations throughout the world.*

**North America  
USA and Canada**  
+1 800 332 3331

**Europe  
France**  
+33 (0)1 60 92 48 34

**Germany**  
+49 (0) 2423 9431 -20  
or -21

**Switzerland**  
+41 56 618 41 11

**United Kingdom**  
+44 1928 534110

**Asia  
Japan**  
+81 3 5826 1615

**China**  
+86-21-68654588  
or +86-10-84193588  
800-810-5118

**India**  
1800 22 8374 (toll-free)  
+91 22 6716 2200

**Thermo Fisher  
Scientific Australia  
Pty Ltd**  
1300 735 292 (free call  
domestic)

**Thermo Fisher  
Scientific New  
Zealand Ltd**  
0800 933 966 (free call  
domestic)

**All Other Enquiries**  
+44 (0) 1928 534 050

### Technical Support

**North America**  
800 332 3331

**Outside North  
America**  
+44 (0) 1928 534 440

[www.thermoscientific.com/chromatography](http://www.thermoscientific.com/chromatography)

©2011 Thermo Fisher Scientific Inc. All rights reserved. All trademarks are the property of Thermo Fisher Scientific Inc. and its subsidiaries. Specifications, terms and pricing are subject to change. Not all products are available in all countries. Please consult your local sales representative for details.

ANCCSCETACNEUT 0611