


Analysis of microcrystalline wax

BPX5

Column part number	054118	Final temperature	375°C, 20 min
Phase	BPX5	Detector	FID
Column	12 m x 0.32 mm x 0.25 µm	Injection mode	On-column
Initial temperature	120°C, 1 min	Carrier gas	H ₂ , 10 psi
Rate	10°C/min		

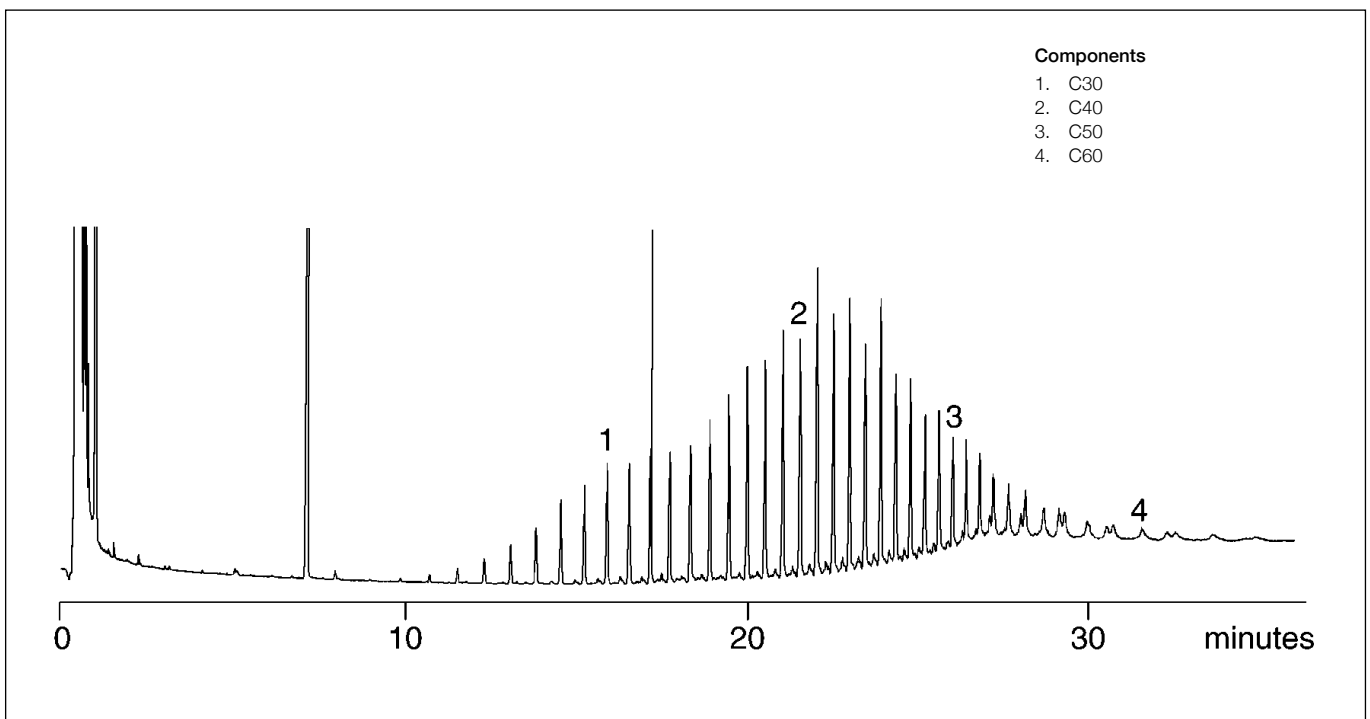

For more information visit www.trajanscimed.com or contact techsupport@trajanscimed.com