


Analysis of argon, oxygen and nitrogen

BP BOND Molsieve 5A

Column part number	0572233		
Phase	BP BOND Molsieve 5A	Final temperature	150°C
Column	25 m x 0.32 mm x 30 µm	Detector	DBD, 150°C
Sample	Argon, oxygen and nitrogen	Carrier gas	He
Initial temperature	60°C, 2 min	Carrier gas flow	30 mL/min
Rate	10°C/min	Injection mode	Split/splitless

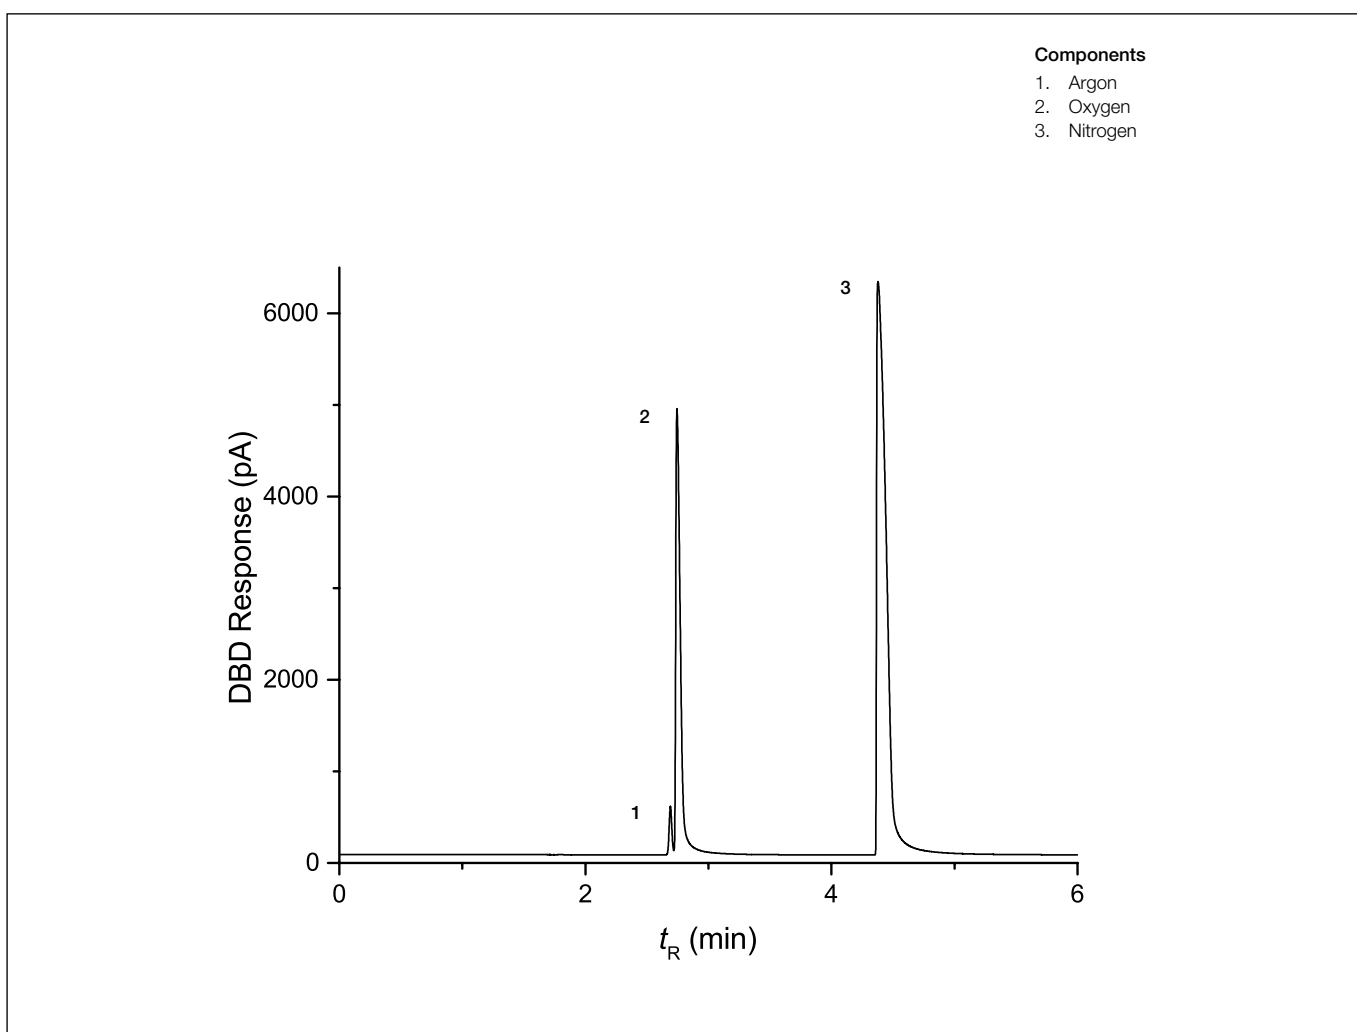

For more information visit www.trajanscimed.com or contact techsupport@trajanscimed.com