

Application Data Sheet

No. 67

GC-MS

Gas Chromatograph Mass Spectrometer

Analysis of Brominated Flame Retardants and Phthalate Esters Under the Same Conditions Using a Pyrolysis GC-MS System (4) - TBBPA and BPBPE -

In recent years, an analysis method has been required to determine not only polybrominated biphenyls (PBBs) and polybrominated diphenyl ethers (PBDEs), which are regulated under the RoHS Directive, but also phthalate esters and other brominated flame retardants not governed by the directive (such as tetrabromobisphenol A (TBBPA), hexabromocyclododecane (HBCDD), and bis(pentabromophenyl)ethane (BPBPE)). TBBPA and BPBPE are not regulated by the RoHS Directive; however, they are frequently detected as brominated flame retardant additives by the EDX screening method. This Application Data Sheet shows the results from analyzing TBBPA and BPBPE in polymers under the same analytical conditions as those in Application Data Sheet 47 using the EGA/PY-3030D Multi-Shot Pyrolyzer and GCMS-QP2020 Ultra systems

Experimental

TBBPA and BPBPE were dissolved with toluene at a concentration of 100 µg/mL, respectively. Polystyrene was dissolved in a mixture of 9:1 (v/v) dichloromethane and xylene at a concentration of 25 mg/mL. 20µL of polystyrene solution (0.5 mg) and 5 µL of each TBBPA and BPBPE solution (0.5 µg) were added to Eco-Cup LF of the pyrolyzer. The solvent was evaporated to dryness at room temperature. The concentration of TBBPA and BPBPE was 1000 ppm in polystyrene. FASST (Fast Automated Scan/SIM Type), which is capable of simultaneous Scan and SIM measurements, was used as the measurement mode. Table 1 shows the analytical conditions and Fig. 1 shows the SIM measurement program.

Table 1: Analytical Conditions

Pyrolysis Instrument	: EGA/PY-3030D Multi-Shot Pyrolyzer		
GC-MS	: GCMS-QP2010 Ultra		
Column	: Ultra ALLOY-PBDE [15 m length, 0.25 mm I.D., df = 0.05 µm]		
[Pyrolyzer]			
Pyrolysis Furnace Temp.	: 200 °C → (20 °C/min) → 300 °C → (5 °C/min) → 340 °C (1 min)		
Interface Temp.	: Manual (300 °C)		
[GC]		[MS]	
Injection Temp.	: 320 °C	Interface Temp.	: 320 °C
Column Oven Temp.	: 80 °C → (20 °C/min) → 300 °C (5 min)	Ion Source Temp.	: 230 °C
Injection Mode	: Split	Solvent Cut Time	: 0.5 min
Carrier Gas	: Helium	Tuning Mode	: Normal
Flow Control Mode	: Constant linear velocity (52.1 cm/sec)	Measurement Mode	: Scan/SIM
Purge Flow Rate	: 3.0 mL/min	Scan Mass Range	: <i>m/z</i> 50 - 1000
Split Ratio	: 50	Scan Event Time	: 0.15 sec
		Scan Speed	: 10,000 <i>u</i> /sec
		SIM Monitoring <i>m/z</i> :	See Fig. 2.
		SIM Event Time	: 0.3 sec
		SIM Micro-Scan Width	: 0.5 <i>u</i>

1 min	Group 1 (No. of <i>m/z</i> channels: 21)	10 min	Group 2 (No. of <i>m/z</i> channels: 11)	16 min
	Tetra-BDE (<i>m/z</i> 325.9, 483.7)		Hexa-BDE (<i>m/z</i> 483.7, 641.5)	
	Penta-BDE (<i>m/z</i> 403.8, 563.6)		Hepta-BDE (<i>m/z</i> 563.6, 721.4)	
	Hexa-BDE (<i>m/z</i> 483.7, 641.5)		Octa-BDE (<i>m/z</i> 641.5, 801.3)	
	Hepta-BDE (<i>m/z</i> 563.6, 721.4)		Nona-BDE (<i>m/z</i> 719.4, 721.4)	
	Tetrabromobisphenol A [TBBPA] (<i>m/z</i> 528.7, 543.7)		Deca-BDE (<i>m/z</i> 799.3, 801.3)	
	Hexabromocyclododecane [HBCDD] (<i>m/z</i> 319.1, 560.6)		Deca-BB (<i>m/z</i> 941.3, 943.3)	
	Diisobutyl phthalate [DIBP] (<i>m/z</i> 149.0, 205.1, 223.1)		Bis(pentabromophenyl)ethane [BPBPE]	
	Di- <i>n</i> -butyl phthalate [DIBP] (<i>m/z</i> 149.0, 205.1, 223.1)		(<i>m/z</i> 484.5, 969.2)	
	Benzylbutyl phthalate [BBP] (<i>m/z</i> 91.0, 149.0, 206.1)			
	Bis(2-ethylhexyl) phthalate [DEHP] (<i>m/z</i> 149.0, 167.0, 279.1)			
	Di- <i>n</i> -octyl phthalate [DOP] (<i>m/z</i> 149.0, 261.1, 279.1)			
	Di-isononyl phthalate [DINP] (<i>m/z</i> 149.0, 167.0, 293.1)			
	Di-isodecyl phthalate [DIDP] (<i>m/z</i> 149.0, 167.0, 307.1)			

Fig. 1: SIM Measurement Program

Results

The chemical structure and mass spectrum of TBBPA are shown in Fig. 2 and 3. Fig. 4 shows the total ion current chromatogram of TBBPA in polystyrene (1000 ppm). The chemical structure and mass spectrum of BPBPE are shown in Fig. 5 and 6. Fig. 7 shows the total ion current chromatogram of BPBPE in polystyrene (1000 ppm).

These analytical conditions can be applied to analyses of PBBs, PBDEs, and phthalate esters. Moreover, using the scan/ SIM mode (FASST) enable accurate determination of target compounds from the SIM data and identification of unknown compounds from the full-scan data.

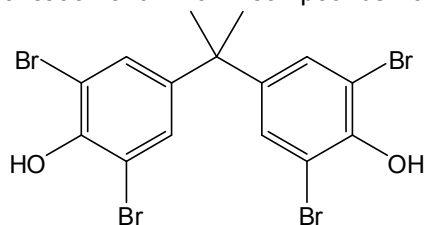


Fig. 2: Compound Structure of TBBPA

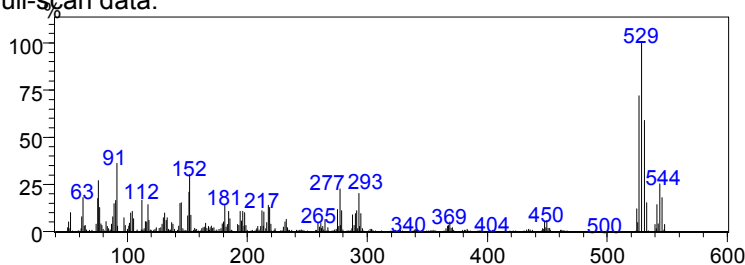


Fig. 3: Mass Spectrum of TBBPA

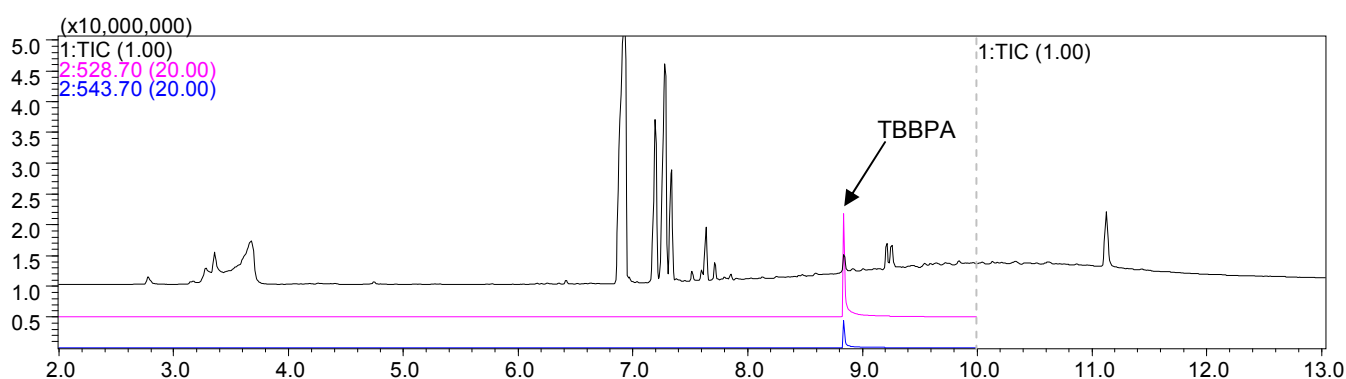


Fig. 4: Total Ion Current Chromatogram of Polystyrene Spiked TBBPA

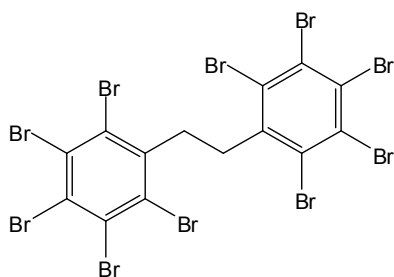


Fig. 5: Compound Structure of BPBPE

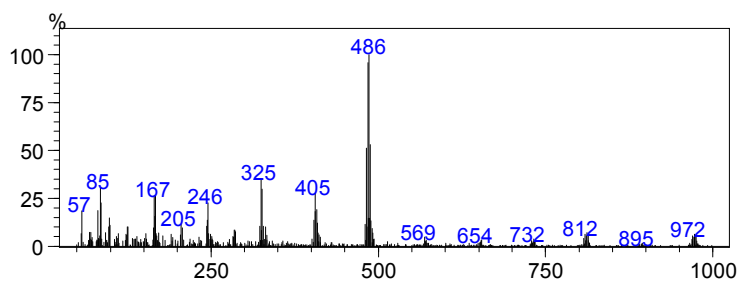


Fig. 6: Mass Spectrum of BPBPE

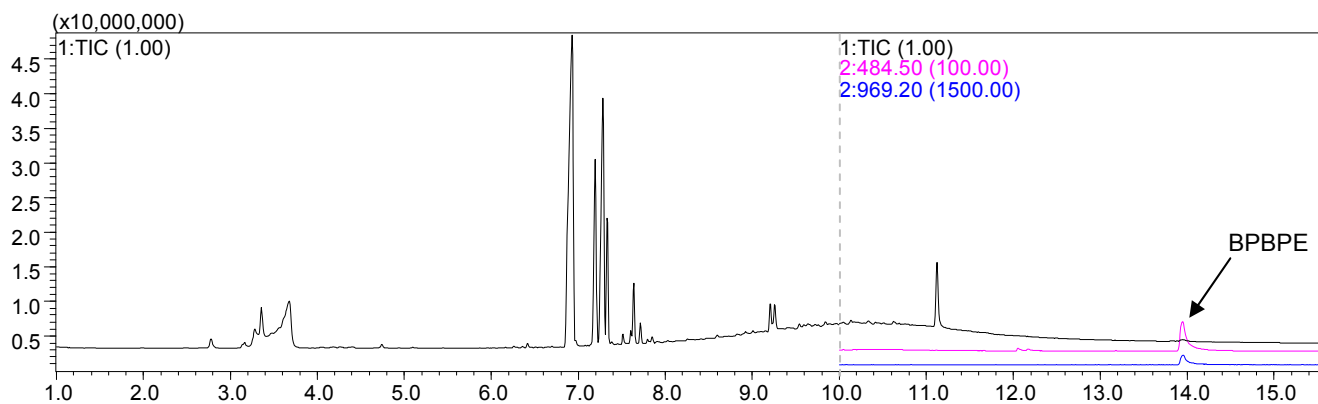


Fig. 7: Total Ion Current Chromatogram of Polystyrene Spiked BPBPE

First Edition: July, 2012