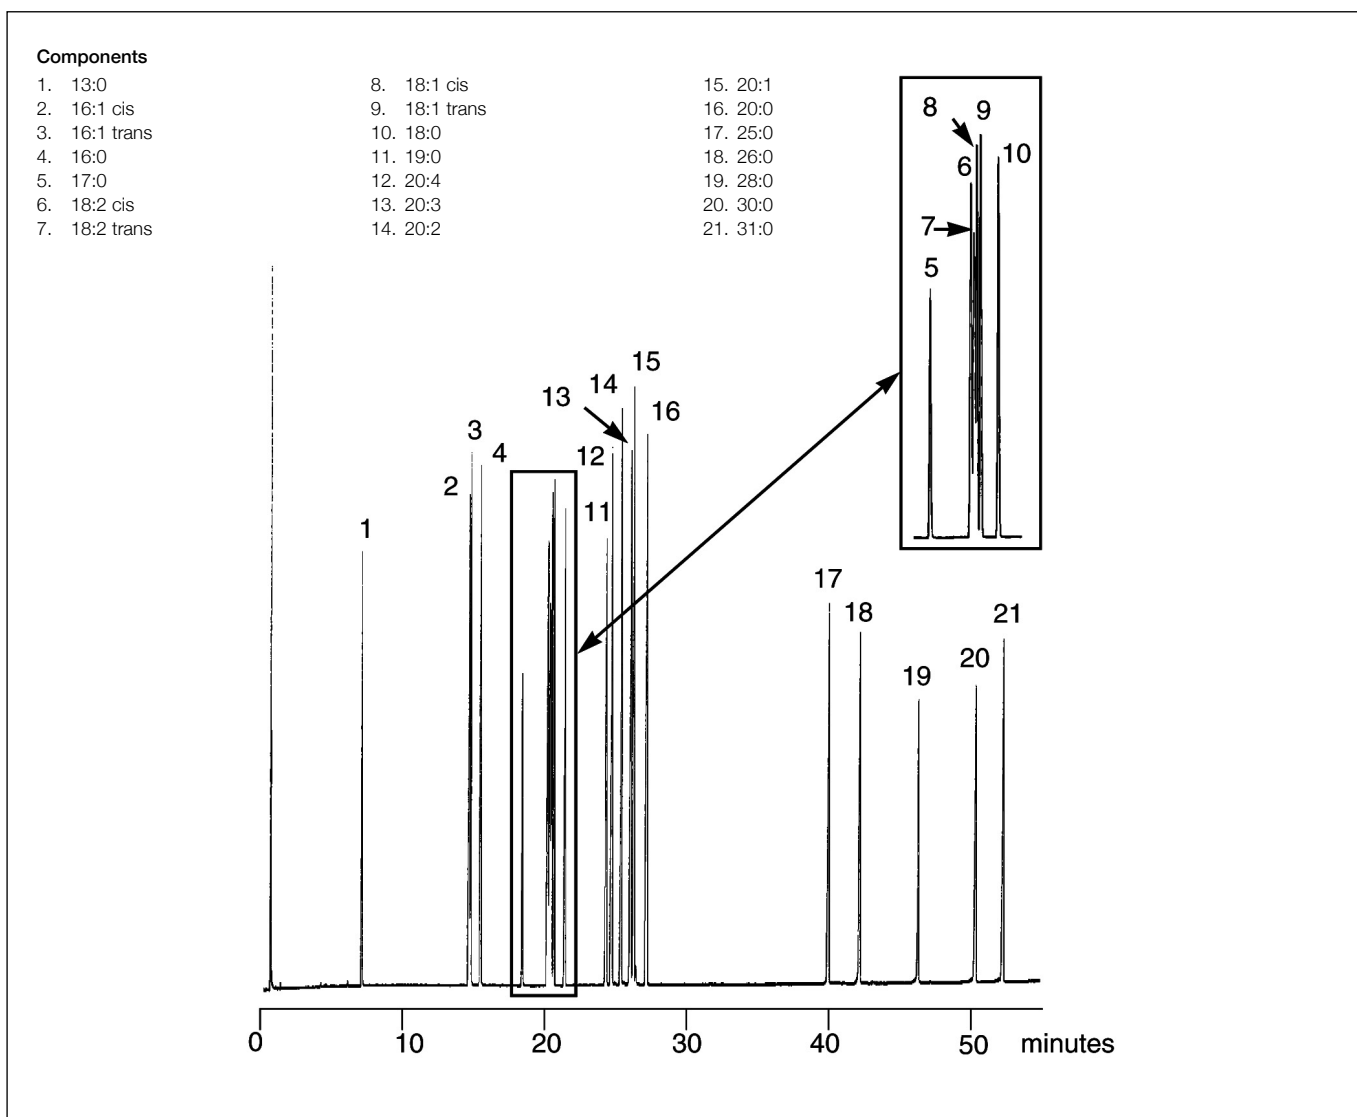


Analysis of fatty acid methyl esters (FAME)

HT5

Column part number	054632		
Phase	HT5	Final temperature	300°C
Column	25 m x 0.22 mm x 0.1 µm	Detector	FID
Initial temperature	120°C	Carrier gas	H ₂ , 10 psi
Rate	3°C/min	Injection mode	Split


 For more information visit www.trajanscimed.com or contact techsupport@trajanscimed.com