


Analysis of mono, di, and triglycerides

BPX5

Column part number	054118		
Phase	BPX5	Final temperature	365°C, 10 min
Column	12 m x 0.32 x 0.25 µm	Detector	FID
Initial temperature	80°C, 1 min	Injection mode	On-column
Rate	10°C/min	Carrier	He, 10 psi

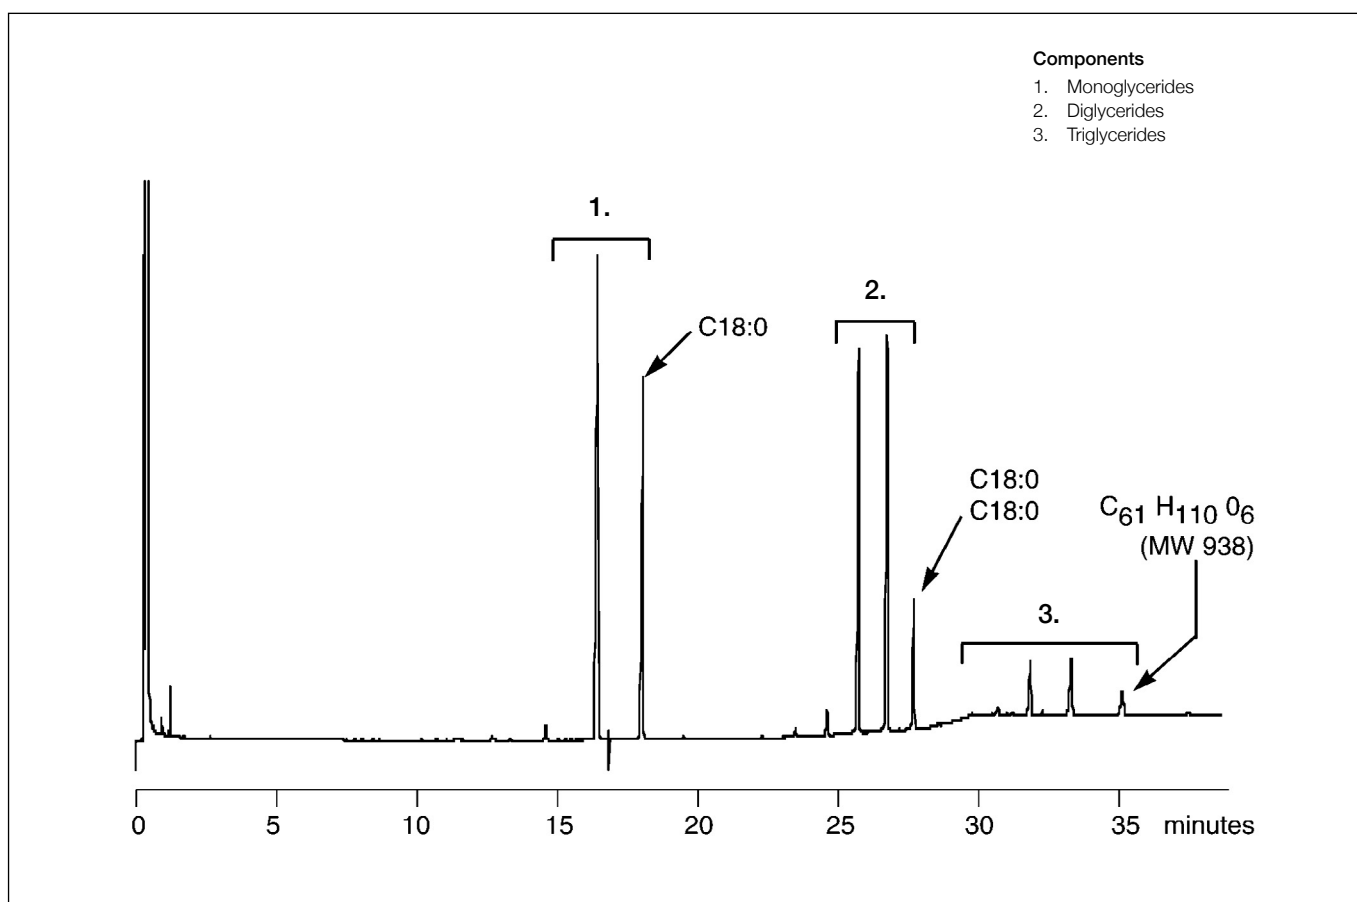

For more information visit www.trajanscimed.com or contact techsupport@trajanscimed.com